


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | X714C

主要用途


APPLICATION

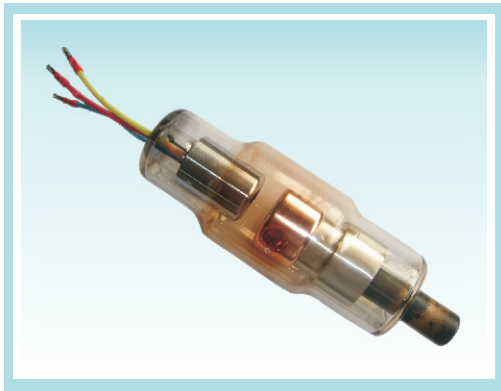

主要供医学诊断X射线机配套使用
It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

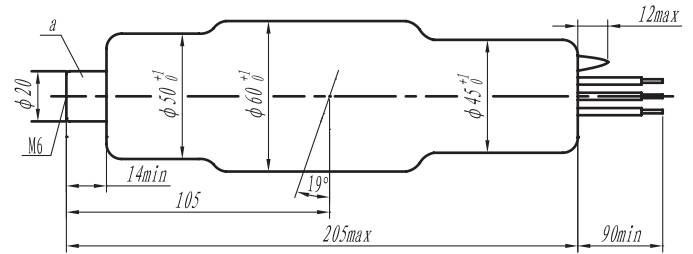


- a* 阳极 anode
- S* 小焦点(红) small focal spot(red)
- C* 公用线(黄) common(yellow)
- L* 大焦点(蓝) large focal spot(blue)

技术参数


TECHNICAL DATA

标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value
	靶材 material	靶面角 angle(°)		
110	W	19	(小焦点) If=4.5A时, Uf=3.7V±0.6V (大焦点) If=4.5A时, Uf=7V±0.8V	1.0/2.6
阳极标称输入功率 nominal anode input power (kW) (1s)	最大连续热耗散 maximum continuous heat dissipation (W)		固有滤过 inherent filtration (mmAl)	质量 weight (kg)
0.8/3.6	250		≤1.0	≤0.9


负载特性曲线 RATING CHARACTERISTICS

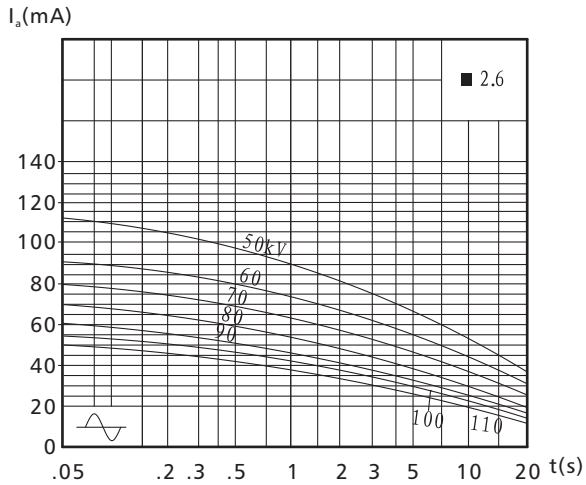

阳极加热冷却特性曲线 ANODE HEATING & COOLING CHARACTERISTICS

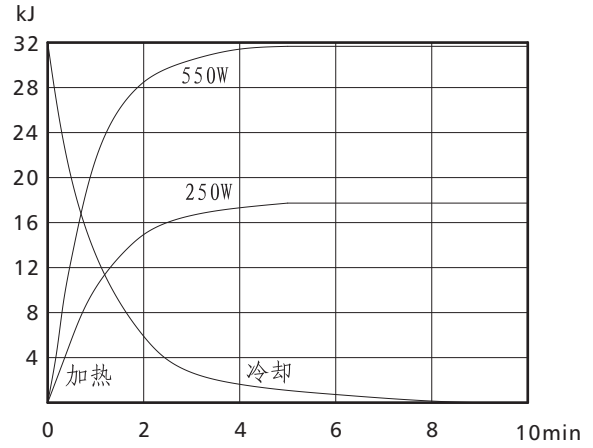

阴极发射特性曲线 CATHODE EMISSION CHARACTERISTIC

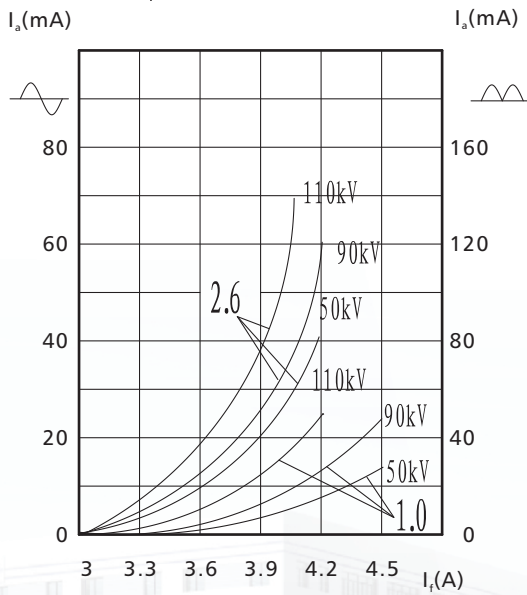

灯丝特性曲线 FILAMENT CHARACTERISTIC

