




诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | X763

主要用途 APPLICATION

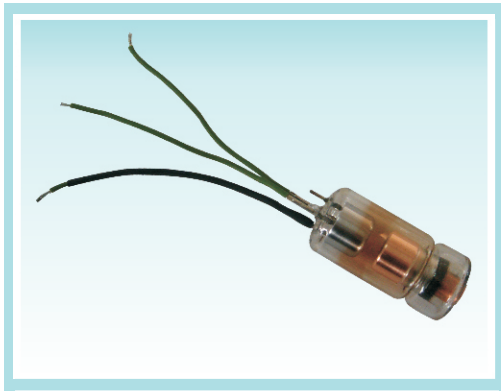

主要供医学诊断X射线机配套使用
It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图 OUTLINE & WIRING DRAWING

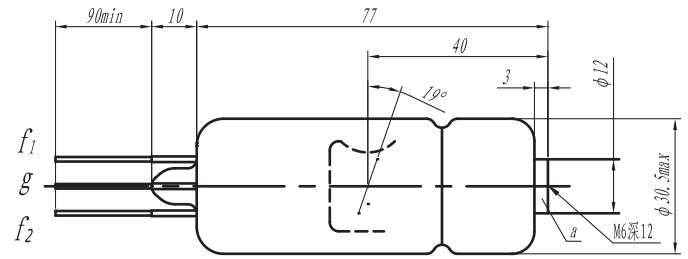

a 阳极 anode
f₁ f₂ 阴极 cathode
g 栅极 grid


技术参数 TECHNICAL DATA

标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value
	靶材 material	靶面角 angle(°)		
70	W	19	If=4.5A时, Uf=6.5V±0.5V	0.7

阳极标称输入功率 nominal anode input power (kW) (1s)	最大连续热耗散 maximum continuous heat dissipation (W)	固有滤过 inherent filtration (mmAl)	栅控电阻 bias resistor (kΩ)	质量 weight (kg)
0.84	90	≤1.0	15≤Rg≤25	≤0.15


负载特性曲线

RATING CHARACTERISTICS

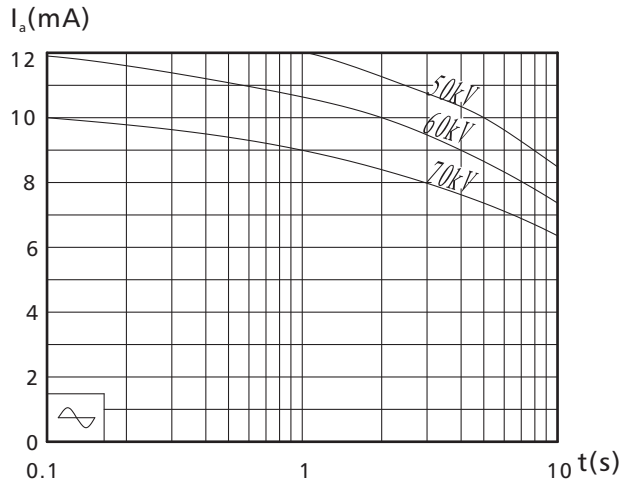


阴极发射特性曲线

CATHODE EMISSION CHARACTERISTIC

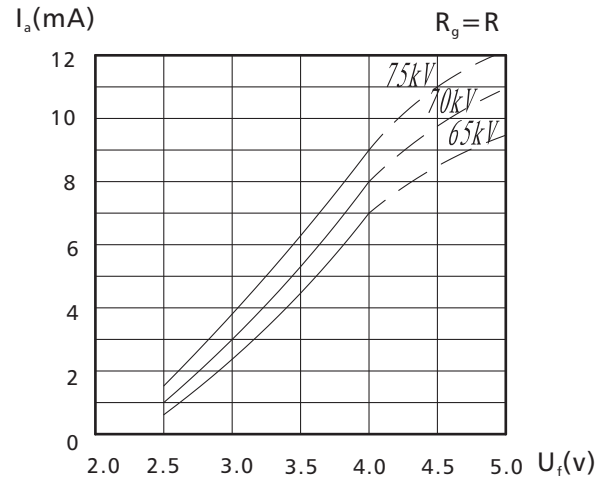

灯丝特性曲线

FILAMENT CHARACTERISTIC

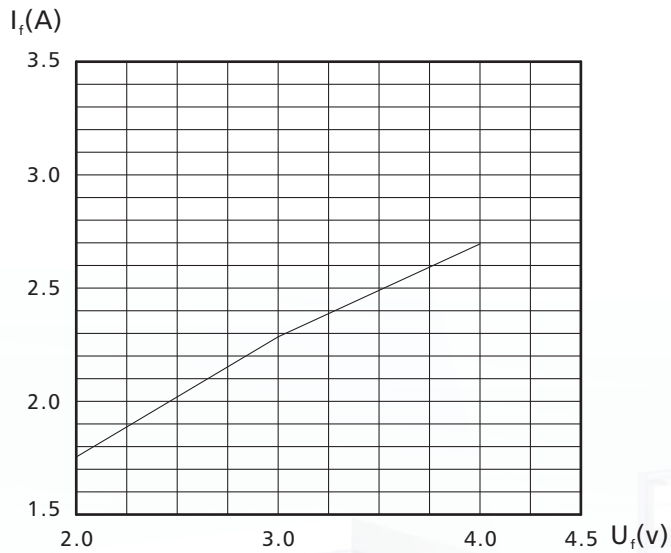

阳极加热冷却特性曲线

ANODE HEATING & COOLING CHARACTERISTICS

