


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | X780

主要用途 APPLICATION



主要供医学诊断X射线机配套使用
It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图 OUTLINE & WIRING DRAWING

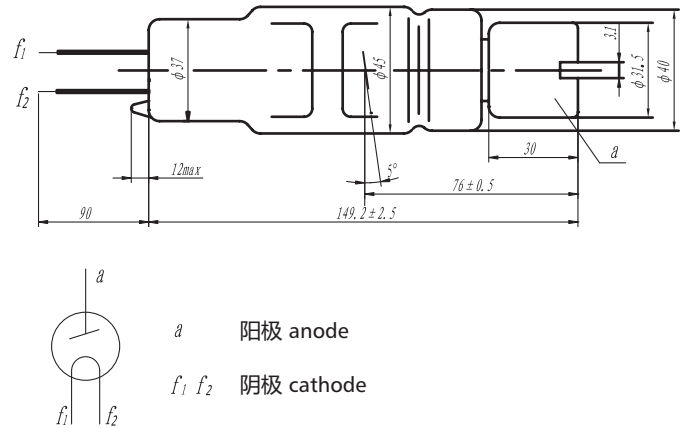


技术参数 TECHNICAL DATA

标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value	质量 weight (kg)
	靶材 material	靶面角 angle(°)			
90	W	5	If=4.5A时, Uf=7V±0.5V	0.6	≤0.6

阳极标称输入功率 nominal anode input power (kW) (1s)	最大连续热耗散 maximum continuous heat dissipation (W)	固有滤过 inherent filtration (mmAl)	阳极最大热容量 maximum anode heat content (kJ)
1.4	225	1.0	35


负载特性曲线

RATING CHARACTERISTICS

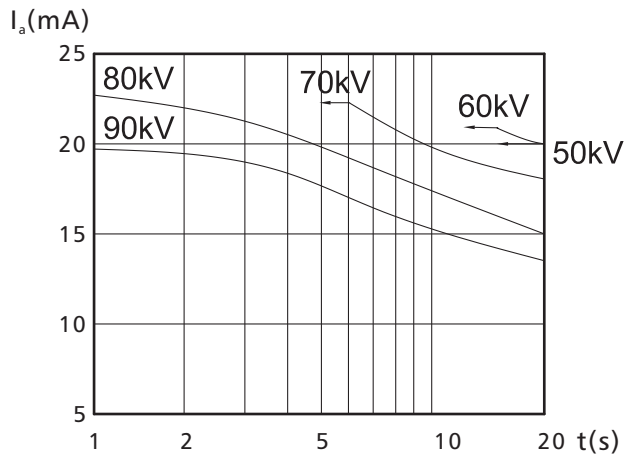

灯丝和阴极发射特性曲线

FILAMENT & CATHODE EMISSION CHARACTERISTIC

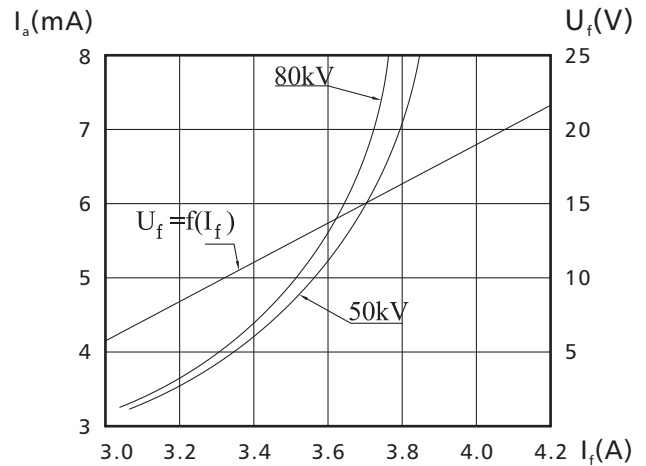

阳极加热冷却特性曲线

ANODE HEATING & COOLING CHARACTERISTICS

