


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | X784

主要用途

APPLICATION

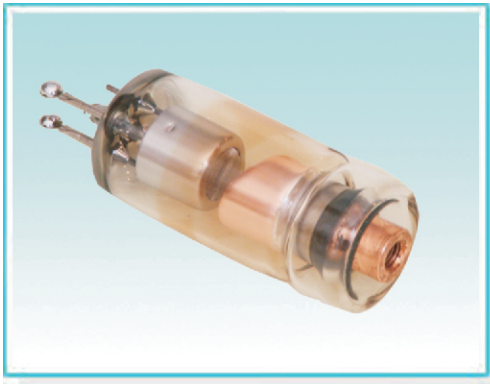


主要供医学诊断X射线机配套使用

It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

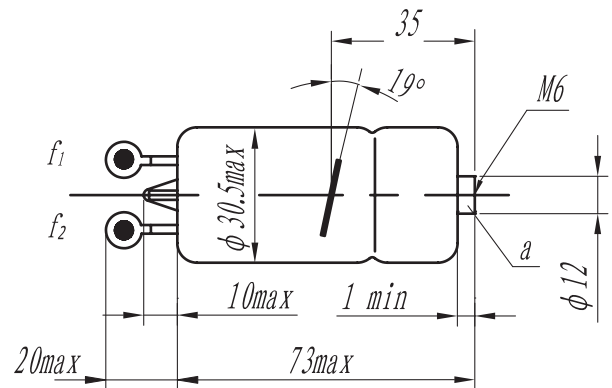

a 阳极 anode

fi f2 阴极 cathode


技术参数

TECHNICAL DATA


标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value	质量 weight (kg)
	靶材 material	靶面角 angle(°)			
70	W	19	I _f =2.5A时, U _f =4V±0.5V	0.4	≤0.12

阳极标称输入功率 nominal anode input power (kW) (1s)	最大连续热耗散 maximum continuous heat dissipation (W)	固有滤过 inherent filtration (mmAl)	阳极最大热容量 maximum anode heat content (kJ)
0.43	100	0.5	4.3


负载特性曲线 RATING CHARACTERISTICS

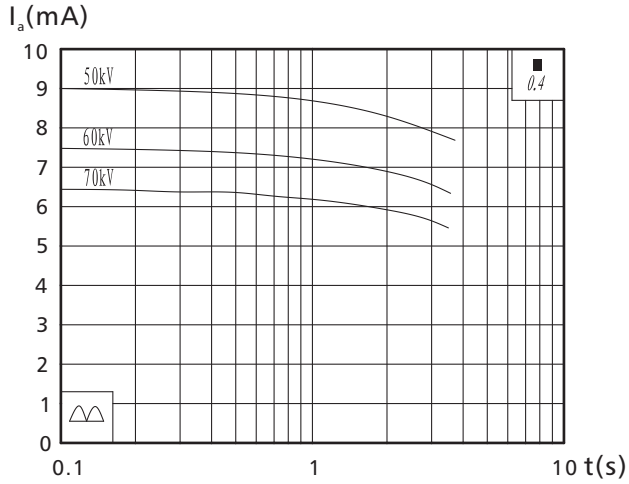

阳极加热冷却特性曲线 ANODE HEATING & COOLING CHARACTERISTICS

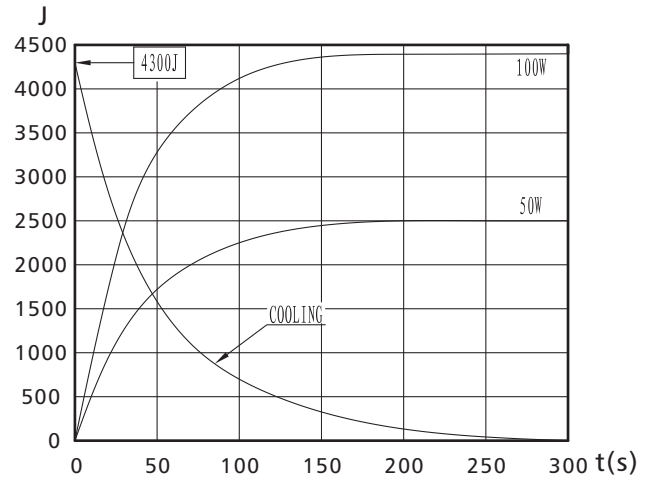

灯丝特性曲线 FILAMENT CHARACTERISTIC

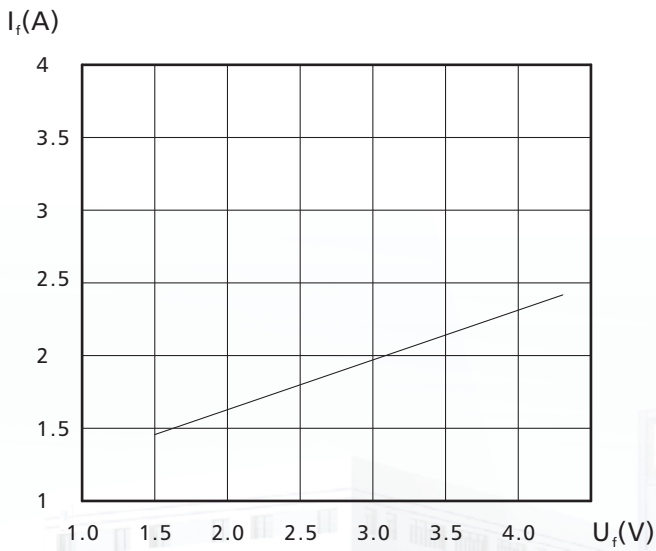

阴极发射特性曲线 CATHODE EMISSION CHARACTERISTIC

