



诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | X791

主要用途 APPLICATION

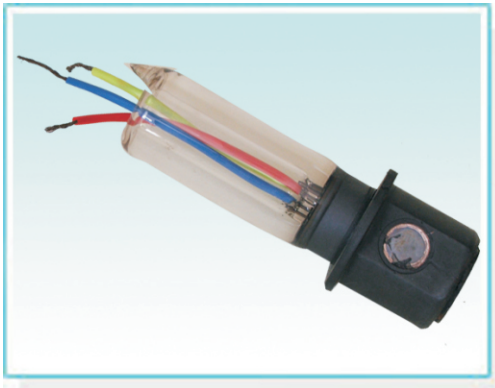

主要供医学诊断X射线机配套使用
It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图 OUTLINE & WIRING DRAWING

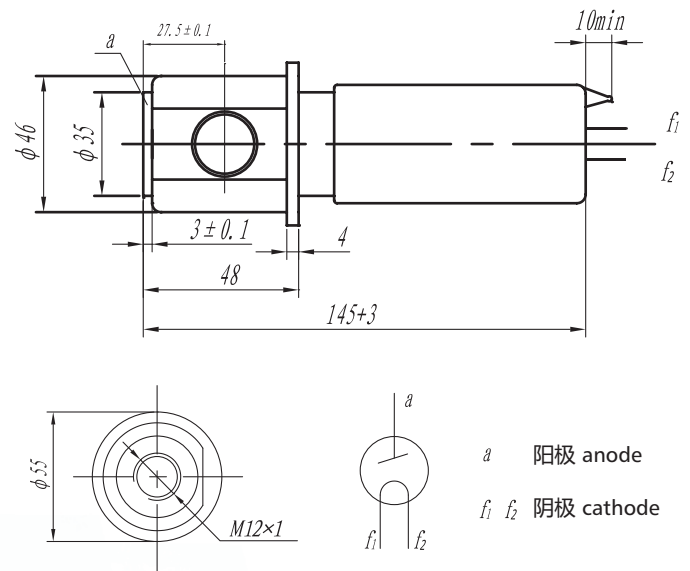

技术参数 TECHNICAL DATA

标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value
	靶材 material	靶面角 angle(°)		
35	Mo	19	(小焦点) $I_f=4A$ 时, $U_f=3.8V \pm 0.4V$ (大焦点) $I_f=4A$ 时, $U_f=3.7V \pm 0.6V$	0.5/1.0
阳极标称输入功率 nominal anode input power (kW) (1s)		固有滤过 inherent filtration (mmAl)		质量 weight (kg)
0.5/1.05		≤ 1.0		≤ 0.7