


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | XD12-0.56/70

主要用途

APPLICATION

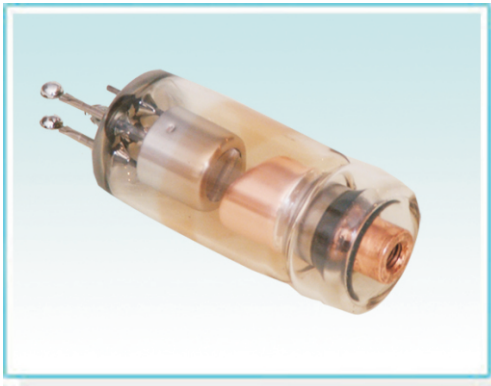


主要供医学诊断X射线机配套使用

It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

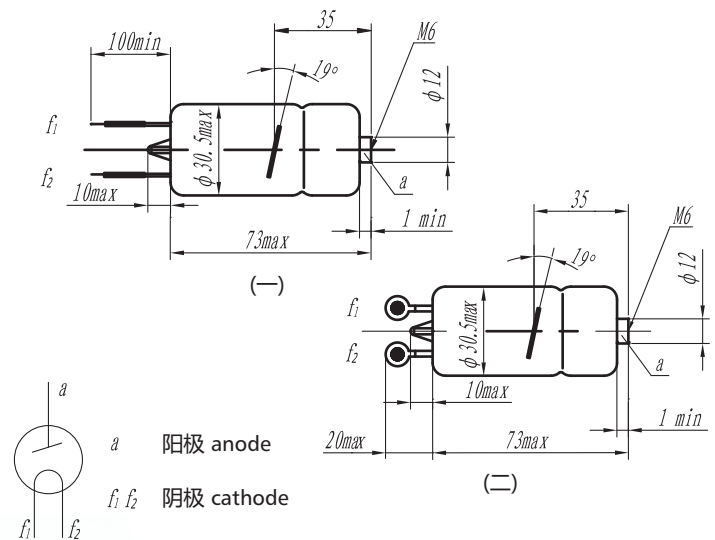

技术参数


TECHNICAL DATA

标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value	质量 weight (kg)
	靶材 material	靶面角 angle(°)			
70	W	19	$I_f = 2A$ 时, $U_f = 3V \pm 0.5V$	0.8	≤ 0.12

阳极标称输入功率 nominal anode input power (kW) (1s)	最大连续热耗散 maximum continuous heat dissipation (W)	固有滤过 inherent filtration (mmAl)	阳极最大热容量 maximum anode heat content (kJ)
0.56	110	0.5	7


负载特性曲线

RATING CHARACTERISTICS

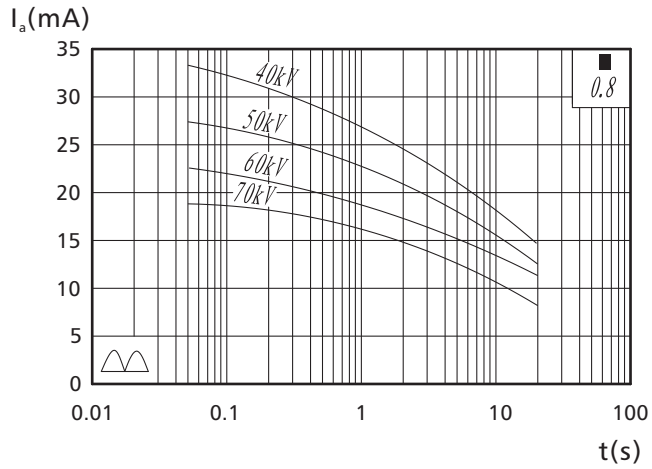


灯丝特性曲线

FILAMENT CHARACTERISTIC

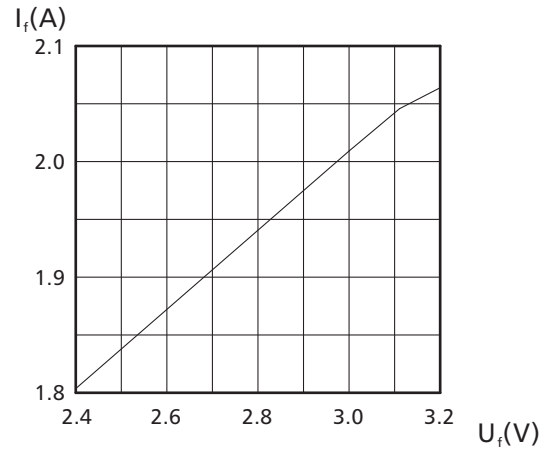

阳极加热冷却特性曲线

ANODE HEATING & COOLING CHARACTERISTICS

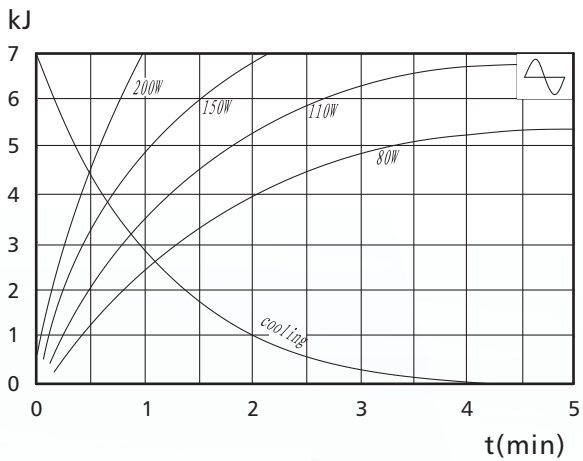

阴极发射特性曲线

CATHODE EMISSION CHARACTERISTIC

