


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | XD2-1.4/85

主要用途



APPLICATION

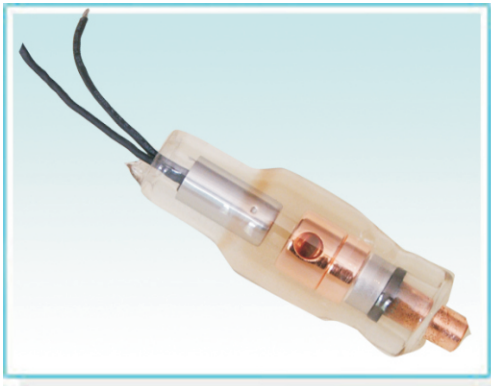

主要供医学诊断X射线机配套使用
It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

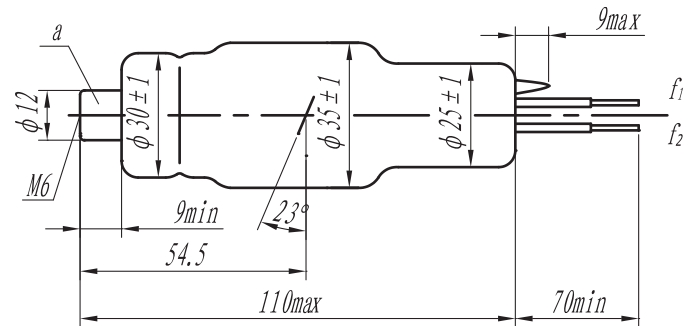

a 阳极 anode

f₁ f₂ 阴极 cathode


技术参数

TECHNICAL DATA


标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value
	靶材 material	靶面角 angle(°)		
85	W	23	I _f =2.5A时, U _f =2.6V±0.7V	1.5

阳极标称输入功率 nominal anode input power (kW) (1s)	固有滤过 inherent filtration (mmAl)	质量 weight (kg)
1.4	≤1.0	≤0.16


负载特性曲线 RATING CHARACTERISTICS

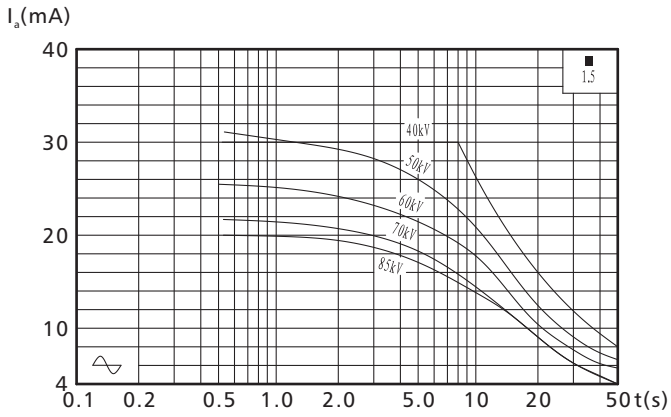

阳极加热冷却特性曲线 ANODE HEATING & COOLING CHARACTERISTICS

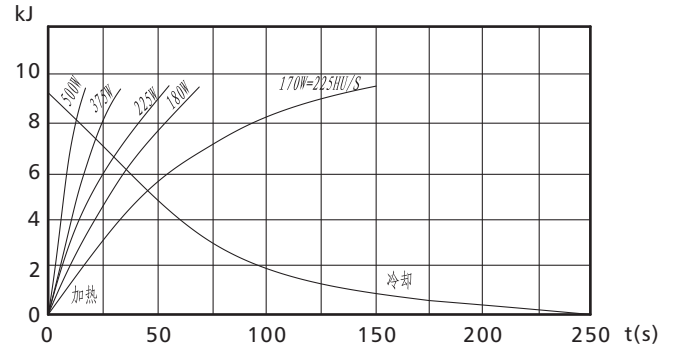

阴极发射特性曲线 CATHODE EMISSION CHARACTERISTIC

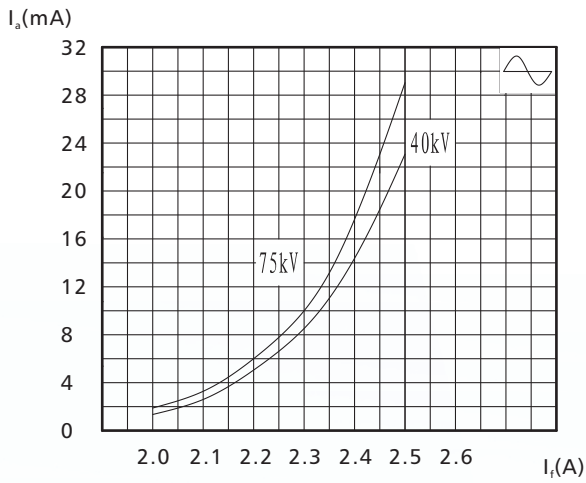

灯丝特性曲线 FILAMENT CHARACTERISTIC

