


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | XD3-3.5/100

主要用途

APPLICATION

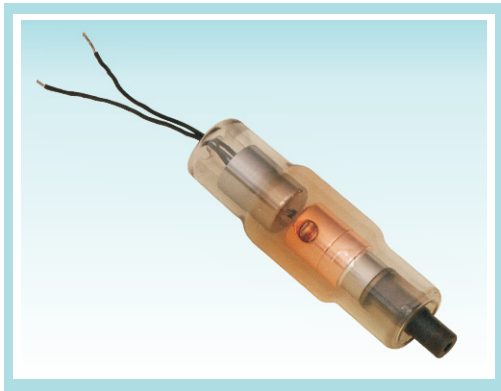


主要供医学诊断X射线机配套使用

It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

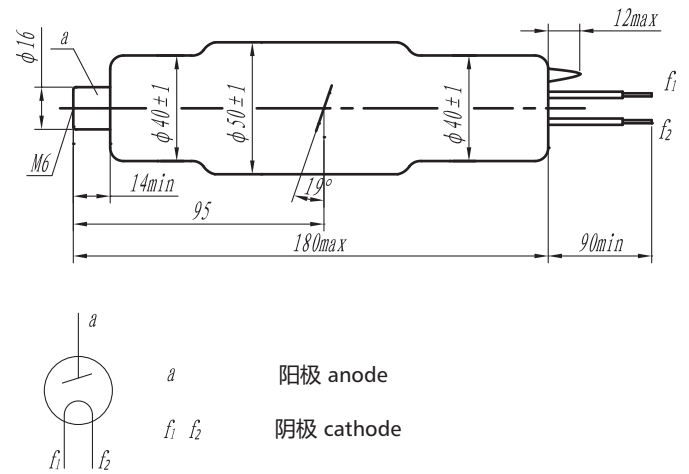


技术参数

TECHNICAL DATA


标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value
	靶材 material	靶面角 angle($^\circ$)		
100	W	19	$I_f = 4.5 \text{ A}$ 时, $U_f = 7 \text{ V} \pm 0.8 \text{ V}$	2.6

阳极标称输入功率 nominal anode input power (kW) (1s)	固有滤过 inherent filtration (mmAl)	质量 weight (kg)
3.5	≤ 1.0	≤ 0.6

负载特性曲线 RATING CHARACTERISTICS

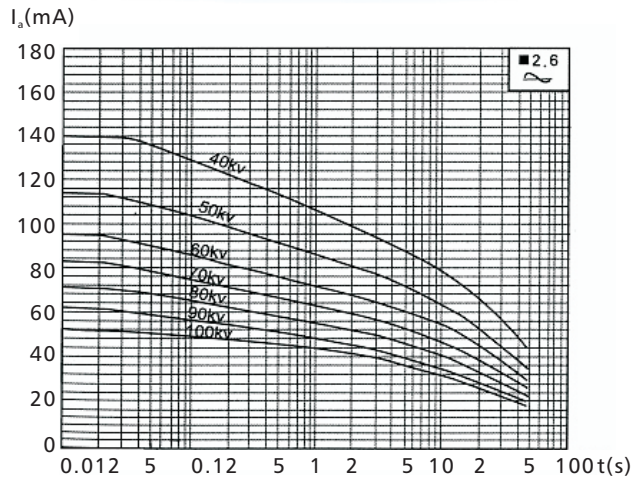

阴极发射特性曲线 CATHODE EMISSION CHARACTERISTIC

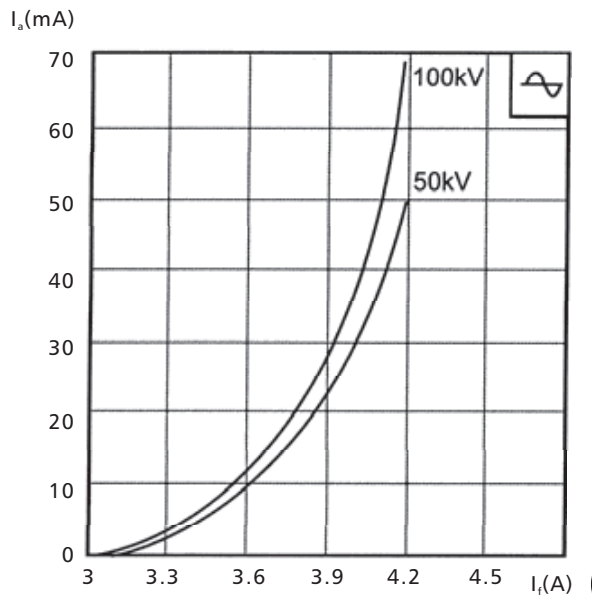

灯丝特性曲线 FILAMENT CHARACTERISTIC

