


诊断用旋转阳极X射线管 执行标准 Standard : YZB/浙 0325 浙食药监械(准)字200第2310204号

管子型号TUBE TYPE XD51-20、40/100 XD51-20、40/125

主要用途

APPLICATION

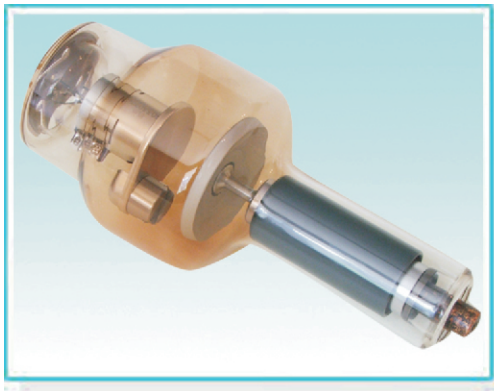


主要供医学诊断X射线机配套使用

It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

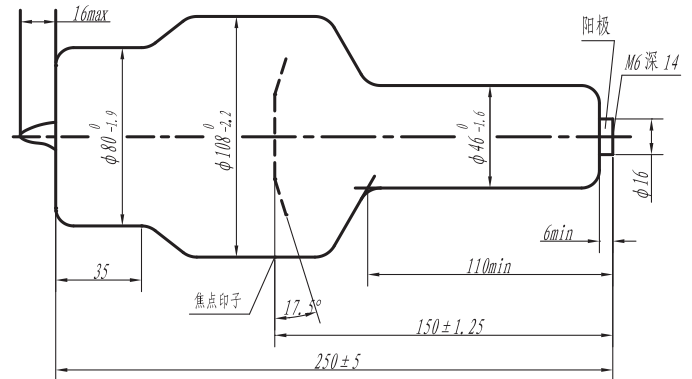

- S 小焦点 Small focal spot
- C 公用线 Common
- L 大焦点 Large focal spot





技术参数

TECHNICAL DATA



标称X射线管电压 nominal X-ray tube voltage(kV)	灯丝特性 filament characteristic	靶 target			阳极转速 anode speed (r/min)
		靶材 material	靶面角 angle(°)	直径 diameter(mm)	
100/125	(小焦点) $I_f=5.5A$ 时, $U_f=7V-9V$	W	17.5	70	2800
	(大焦点) $I_f=5.5A$ 时, $U_f=10V-13V$				

固有滤过 inherent filtration (mmAl)	质量 weight (kg)	焦点标称值 nominal focal spot value	阳极标称输入功率 nominal anode input power (kW) (0.1s)	阳极最大热容量 maximum anode heat content(kJ)	最大连续热耗散 maximum continuous heat dissipation(W)
0.8-1.2	≤1.5	1.0/2.0	20/40	100(140kHU)	410

负载特性曲线 RATING CHARACTERISTICS

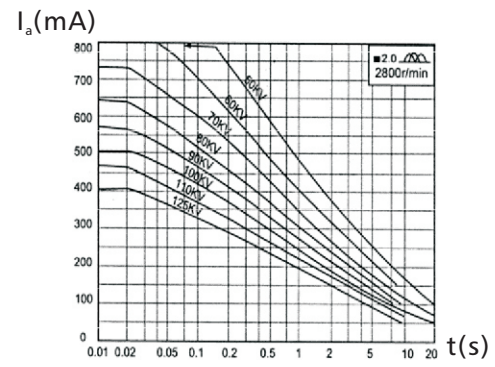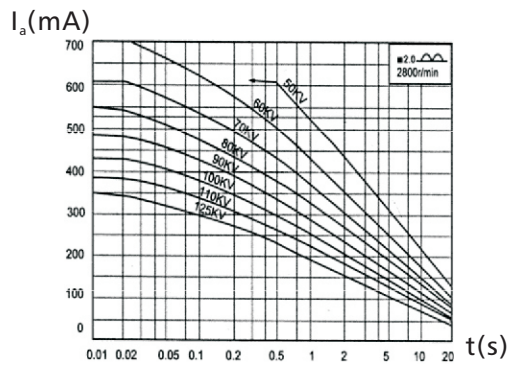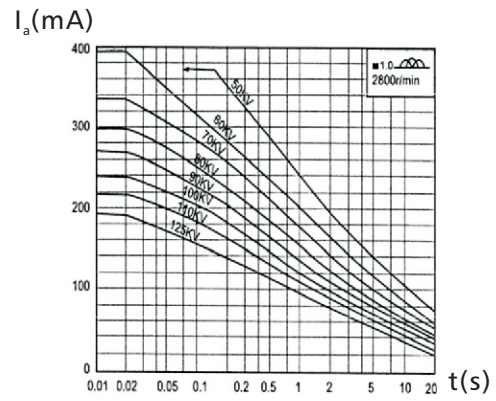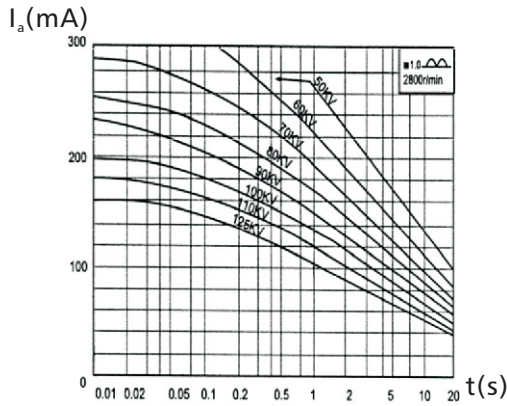

灯丝和阴极发射特性曲线 FILAMENT & CATHODE EMISSION CHARACTERISTIC

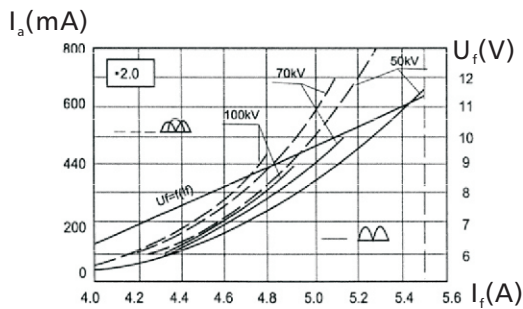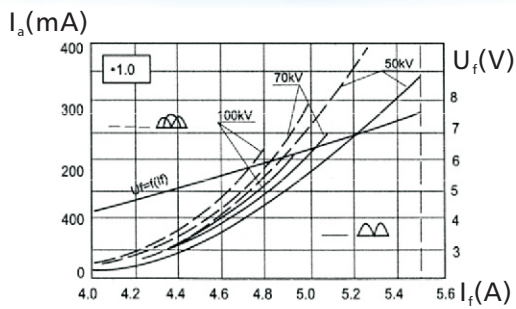

阳极加热冷却特性曲线 ANODE HEATING & COOLING CHARACTERISTICS

