


诊断用固定阳极X射线管 | 执行标准 Standard : YZB/浙 0326 浙食药监械(准)字200第2310012号
管子型号TUBE TYPE | XD9-4/100

主要用途



APPLICATION

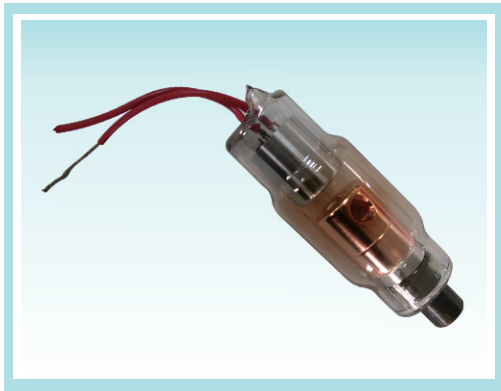

主要供医学诊断X射线机配套使用
It is designed for main applications used in x-ray equipment for medical diagnosis

外形与接线图

OUTLINE & WIRING DRAWING

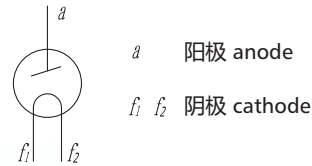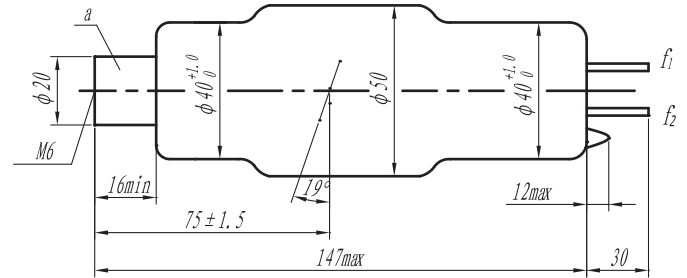



技术参数

TECHNICAL DATA


标称X射线管电压 nominal X-ray tube voltage (kV)	靶 target		灯丝特性 filament characteristic	焦点标称值 nominal focal spot value
	靶材 material	靶面角 angle(°)		
100	W	19	I _f =4A时, U _f =6.8V±0.7V	2.2

阳极标称输入功率 nominal anode input power (kW) (1s)	固有滤过 inherent filtration (mmAl)	质量 weight (kg)
4	≤1.0	≤0.6

负载特性曲线 RATING CHARACTERISTICS

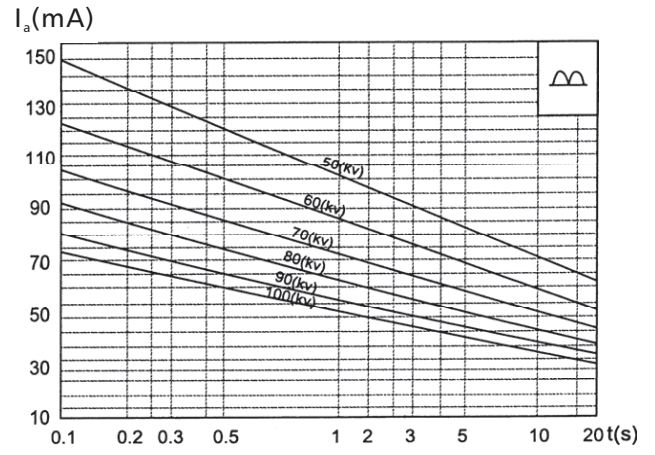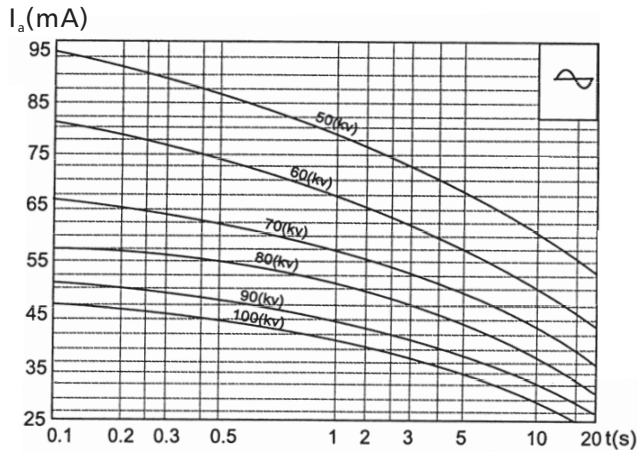

灯丝和阴极发射特性曲线 FILAMENT & CATHODE EMISSION CHARACTERISTIC

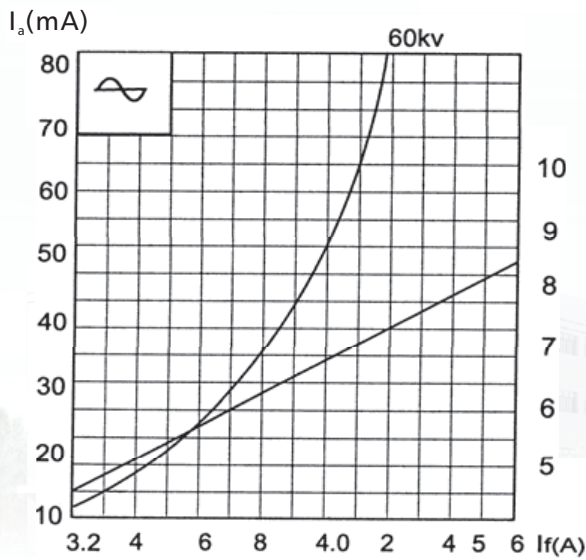

阳极加热冷却特性 ANODE HEATING & COOLING CHARACTERISTICS

